

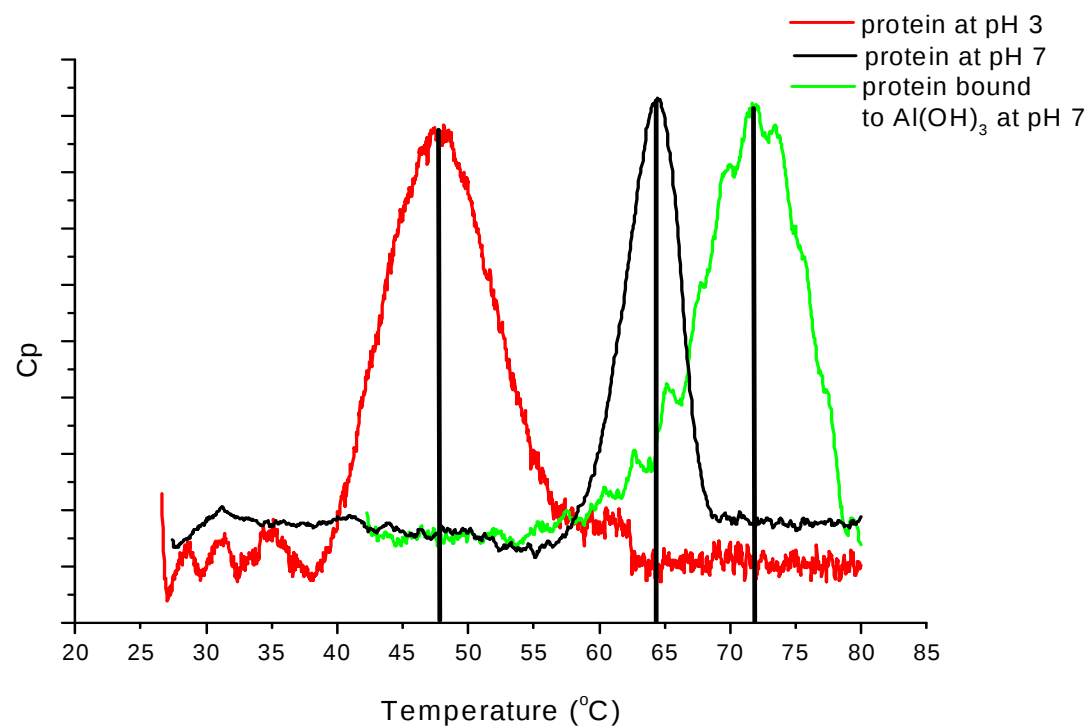


Figure S13: Secondary structure analysis of a recombinant vaccine antigen candidate (100 $\mu\text{g/ml}$) by differential scanning calorimetry formulated at pH 7 and pH 3 with and without aluminium hydroxide adjuvant.